

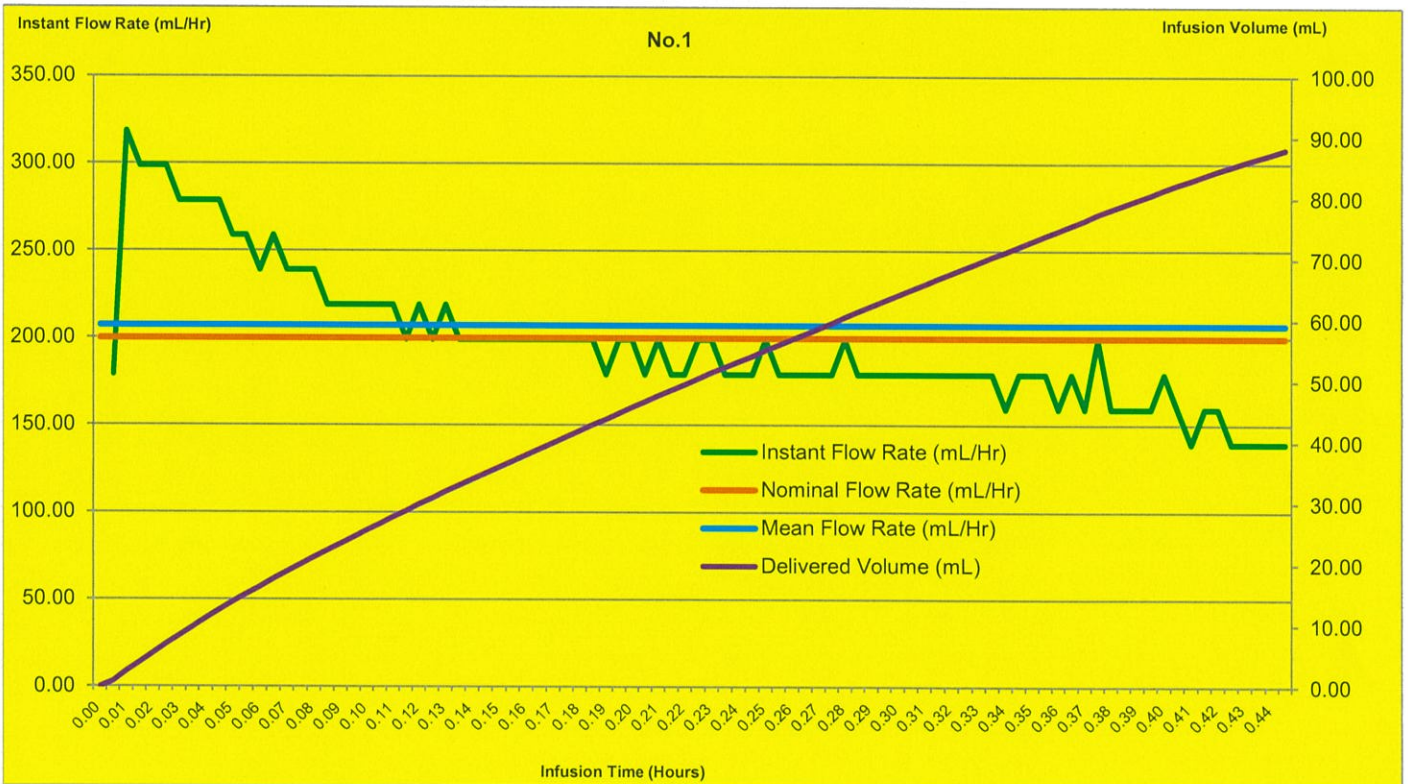
Doc. No.: FM-TM-011-01		Title: Flow Rate Test Report	
Rev. 01	CCR-14-11-001	Effective Date: 2014-11-03	Page 1 of 4

1. Product Identification

Article Number	481010	Nominal Flow Rate (mL/Hr)	200
Article Name	SMARTez 100-200-30m	Nominal Volume (mL)	100
Batch No.	S20E26	Nominal Time (Hr)	0.5
EO Sterilization	<input type="checkbox"/> Before <input checked="" type="checkbox"/> After	Test Date	2020-09-01
Equipment	Load Cell	Room Temperature (°C)	20.6
Solution	Nacl 0.9% (Normal Saline)	Result	PASS

2. Result Summary

Sample No.	Load Cell No.	Mean Flow Rate		Volume delivered at an instantaneous flow rate within ±50% of the nominal flow rate		Result
		Mean Flow Rate (mL/Hr)	Deviation from Nominal Flow Rate (Spec: ±15%)	Volume (mL)	Percentage of Nominal Volume (Spec: ≥80%)	
1	No.1	207.27	3.63%	88.29	88.29%	PASS

3. Infusion Volume & Instant Flow Rate Chart

4. Remark: Profile using Load cell.

Tested By: Malimam
Date: 2020-09-01
Verified By: [Signature]
Date: 2020-09-01